

TEST REPORT

(Electronic version)



No: 200180842

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: GNVY-2443-14

ISSUE DATE: 2020-06-28

扫码下载报告



APPLICANT: SIAM GLOBAL GROUP CO., LTD
ADDRESS: 253/1038 SOI KHEHAROMKLAO 64, KWANG KLONGSONGTONNUN, KHET LATKRABANG, BANGKOK
10520 THAILAND

INFORMATION CONFIRMED BY APPLICANT:

YAMADA VALVED FOLDABLE KN95 MASK

QUANTITY: 30 PIECES

BRAND: YAMADA

LOT NO. : 8242

DATE RECEIVED/DATE TEST STARTED: 2020-06-19

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
VISUAL FIELD	M
HEAD BAND	M
EXHALATION VALVE COVER	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200180841.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200180842

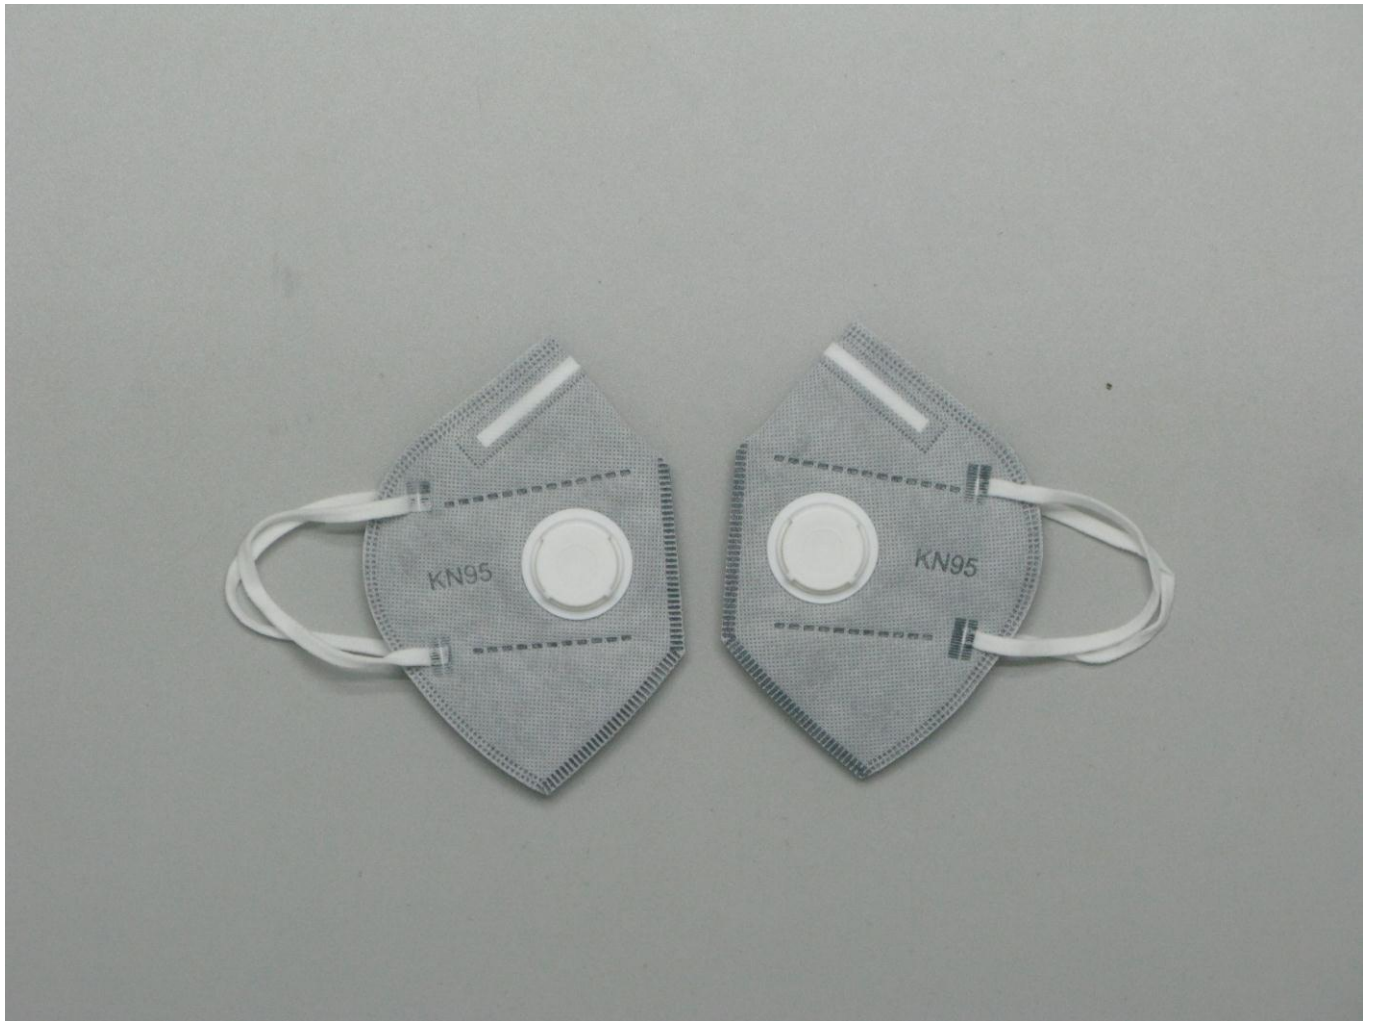

TEST REPORT

(Electronic version)

No:200180842

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(%)

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³, TEMP:23.8℃ RH:36.5%)

FILTRATION EFFICIENCY: UNTREATED SAMPLE

1# 99.270
2# 99.148
3# 99.075
4# 99.172
5# 98.92
6# 98.47
7# 99.025
8# 98.85
9# 98.63
10# 99.011

CONDITIONING TREATED

1# 99.233
2# 98.76
3# 97.98
4# 98.49
5# 99.014

REQUIREMENT

FILTRATION EFFICIENCY:
≥95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 157.2
2# 159.6

PRETREATMENT SAMPLE:

1# 143.1
2# 145.6

REQUIREMENT

≤350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 90.7
2# 93.9

PRETREATMENT SAMPLE:

1# 82.4
2# 84.7

REQUIREMENT

≤250
(GB 2626-2006)

VISUAL FIELD(°)

(GB 2890-2009 6.8)

65

REQUIREMENT

≥60
(GB 2626-2006)

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUSTING PARTS OF MASK SHOULD NOT SLIP OR BREAK UNDER 10N TENSION FOR 10S.
(GB 2626-2006)



PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200180842

EXHALATION VALVE COVER
(GB 2626-2006 6.8)

UNTREATED SAMPLE:	REQUIREMENT
1# PASS	EXHALATION VALVE COVER OF MASK SHOULD
2# PASS	NOT SLIP, BREAK OR DEFORM UNDER 10N
3# PASS	AXIAL TENSION FOR 10S. (GB 2626-2006)



————End of Report————

PAGE 4 OF 4